



NATIONAL TYPE EVALUATION PROGRAM

Certificate of Conformance

for Weighing and Measuring Devices

For:

Non-Computing Scale
Postal Weight Classifier, Digital Electronic
Model: BC
 n_{\max} : 5600
 e_{\min} : 0.05 lb / 0.1 oz / 0.005 kg
Capacity: 7 lb to 300 lb (3 kg to 150 kg)
Platform: 12 in x 14 in – 16 in x 20 in
Accuracy Class: III

Submitted By:

Mettler-Toledo, LLC
1150 Dearborn Drive
Worthington, Ohio 43085
Tel: 614-438-4387
Fax: 614-438-4355
Contact: Scott Davidson
Email: scott.davidson@mt.com
Web site: www.mt.com

Standard Features and Options**Standard Features:**

- Semi-Automatic (push button) Zero Setting Mechanism (SAZSM)
- Automatic Zero Tracking (AZT)
- Initial Zero Setting Mechanism (IZSM)
- Semi-Automatic (push button) Tare
- Units Switching Capability (lb, kg, g, lb/oz)
- Multiple Range and Multi-Interval Capability
- Liquid Crystal Display (LCD)
- AC/DC Adapter (scale may also be powered via USB port)
- Weight Classifier Mode (For Postal Use)
- USB, serial communication interface for data output to host system

Load Cells Used:

- Mettler Toledo, model 0785, 0795 (non-NTEP) and model MT1041 (NTEP CC 11-088) or NTEP Certified Compatible and equivalent

Temperature Range: 0 °C to 40 °C (32 °F to 104 °F)

This device was evaluated under the National Type Evaluation Program and was found to comply with the applicable technical requirements of "NIST Handbook 44: Specifications, Tolerances and Other Technical Requirements for Weighing and Measuring Devices." Evaluation results and device characteristics necessary for inspection and use in commerce are on the following pages.

John Gaccione
Chairman, NCWM, Inc.

Stephen Benjamin
Chairman, National Type Evaluation Program Committee
Issued: May 21, 2014

1135 M Street, Suite 110 / Lincoln, Nebraska 68508

The National Conference on Weights and Measures (NCWM) does not approve, recommend or endorse any proprietary product or material, either as a single item or as a class or group. Results shall not be used in advertising or sales promotion to indicate explicit or implicit endorsement of the product or material by the NCWM.



Mettler-Toledo, LLC


Non-Computing Scale / BC

Application: The scale is suitable for weighing letters or parcels for delivery by the U.S. Postal Service or private shipping companies. In a commercial application the requirements for the displayed weight and the weighing operation is to be visible by the customer can be satisfied by equipment positioning and the use of an optional remote weight display. The scale shall be marked with the words "WEIGHT CLASSIFIER FOR POSTAL USE" when used as a weight classifier.

Identification: The required information is on an adhesive badge located on the base unit. It is visible by removing the scale platter.

Sealing: The scale can be sealed with a wire security seal threaded through a plug and a tab on the base, and a screw head to a tab on the cover plate, which secures the access to the metrological switch. This prohibits modification to the set-up and calibration features on the electronic circuit board assembly.

Top of scale under platter

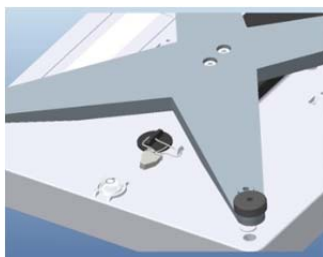

Bottom of scale



Test Conditions: This Certificate supersedes Certificate of Conformance 13-111 and is issued to increase the capacity to 300 lb (150 kg) and include a larger platter size of 16 in x 20 in. Two model BC were submitted (300 lb x 0.1 lb and 150 kg x 0.05 kg) for evaluation. Several increasing/decreasing load and shift tests were performed. A discrimination zone of uncertainty test and suitability of level indicator test was performed. Also, a power supply of 100 VAC and 240 VAC and 5 VDC was applied to the scale. The devices were tested over a temperature range of 0 °C to 40 °C (32 °F to 104 °F). A load of approximately one-half scale capacity was applied to the scales over 100 000 times. The scales was tested periodically during this period. The shift and discrimination zone of uncertainty tests were repeated after the permanence test. The previous test conditions are listed below for reference.

Certificate of Conformance 13-111: The emphasis of the evaluation was on the device design, operation, performance, and compliance with influence factor requirements. One model BC multiple range (10/100 lb x 0.1/0.5 oz), one model BC multi-interval (7/70 lb x 0.1/0.2 oz), one model BC single range (30 kg x 0.01kg) and one model BC (150 lb x 0.05 lb) were submitted for evaluation. Several increasing/decreasing load and shift tests were performed. A discrimination zone of uncertainty test and suitability of level indicator test was performed. Also, a power supply of 100 VAC and 240 VAC was applied to the scale. The device was tested over a temperature range of 0 °C to 40 °C (32 °F to 104 °F). A load of approximately one-half scale capacity was applied to the scale over 100 000 times. The scale was tested periodically during this period. The shift and discrimination zone of uncertainty tests were repeated after the permanence test.

Evaluated By: T.Buck (OH) 13-111, 13-111A1

Type Evaluation Criteria Used: : NIST Handbook 44 Specifications, Tolerances, and Other Technical Requirements for Weighing and Measuring Devices, 2014 Edition. NCWM Publication 14 Weighing Devices, 2014 Edition.

Conclusion: The results of the evaluation and information provided by the manufacturer indicate the device complies with applicable requirements.

Information Reviewed By: J. Truex (NCWM) 13-111, 13-111A1



Mettler-Toledo, LLC
Non-Computing Scale / BC

Examples of Device:

